



Pulse Sequences

Application Brochure

MAGNETOM Avanto, Espree, Symphony a Tim System,
Trio a Tim System, Verio

www.siemens.com/healthcare

SIEMENS

Pulse Sequences

Application Brochure

MAGNETOM Avanto, Espree, Symphony a Tim System,
Trio a Tim System, Verio

This brochure informs the user about the pulse sequences of *syngo* MR for the MR tomographs listed on the front page. It addresses medical personnel working in the area of MR tomography.

Contents

Basics	Overview	2
	Sequence variants	4
	Sequence variant components (I)	6
	Sequence variant components (II)	8
	Sequence nomenclature (I)	10
	Sequence nomenclature (II)	12
Tim	Spin echo with fixed temporal	
Application	sequence, sequence description	14
Suite	Spin echo with optimized temporal	
	sequence, sequence description	16
	Spin echo with optimized temporal	
	sequence, parameter ranges	18
	Turbo spin echo,	
	sequence description (I)	20
	Turbo spin echo,	
	sequence description (II)	22
	Turbo spin echo,	
	sequence description (III)	24
	Turbo spin echo,	
	sequence description (IV)	26

Turbo spin echo, parameter ranges (I)	28
Turbo spin echo, parameter ranges (II)	30
Gradient echo, sequence description (I)	32
Gradient echo, sequence description (II)	34
Gradient echo, parameter ranges (I)	36
Gradient echo, parameter ranges (II)	38
Steady-state gradient echo, sequence description	40
Gradient echo for inflow angiography (ToF), sequence description	42
Contrast-enhanced angiography, sequence description	44
Contrast-enhanced angiography, parameter ranges (I)	46
Contrast-enhanced angiography, parameter ranges (II)	48

Contents

Rephased-dephased angiography, sequence description	50
Inflow angiography (ToF), sequence description	52
Phase-contrast angiography, sequence description	54
Fast dynamic imaging, sequence description	56
TrueFISP, sequence description (I)	58
TrueFISP, sequence description (II)	60
TrueFISP, sequence description (III)	62
TrueFISP, sequence description (IV)	64
TrueFISP, sequence description (V)	66
TrueFISP, sequence description (VI)	68
TrueFISP, sequence description (VII)	70

	EPI sequences, sequence description	72
	EPI sequences, parameter ranges	74
CISS & DESS	Sequence description	76
TGSE	Sequence description	78
	Parameter ranges	80
AutoAlign	Sequence description	82
Advanced Cardiac	Sequence description (I)	84
	Sequence description (II)	86
	Sequence description (III)	88
	Sequence description (IV)	90
	Sequence description (V)	92
	Sequence description (VI)	94
	Sequence description (VII)	96
	Sequence description (VIII)	98
	Sequence description (IX)	100
	Sequence description (X)	102
	Sequence description (XI)	104

Contents

Flow	Sequence description	106
Quantification	Parameter ranges	108
Diffusion	Sequence description	110
	Parameter ranges	112
Perfusion	Sequence description	114
BOLD	Sequence description (I)	116
	Parameter ranges	118
	Sequence description (II)	120
Interactive	Sequence description	122
Realtime	Parameter ranges	124
SWI	Susceptibility-Weighted Imaging	126
BLADE	Application/sequence description	128
	Sequence parameters	130
	Application notes	132
tse Dixon	Application	134
	Sequence description/ sequence parameters	136

SPACE	Application	138
	Sequence description/protocols	140
	Sequence parameters	142
TimCT	Sequence description	144
Angiography		
MR thermo-	Sequence description	146
metry		

Overview

The MR system is equipped with optimized pulse sequences that allow for highly flexible adjustments to meet your clinical requirements.

Parameter ranges	The sequences cover a broad range of parameters and allow for flexible timing (exception: flow-compensated spin echo sequences that have a slightly limited parameter range).
-------------------------	---

Application packages


The sequences described in this brochure are part of the following application packages:

- Tim Application Suite
- CISS & DESS
- TGSE
- AutoAlign
- Advanced Cardiac
- Flow Quantification
- Inline Diffusion Imaging
- Inline Perfusion Imaging
- Inline BOLD Imaging
- Advanced Functional Neuro
- Interactive Realtime
- Susceptibility-Weighted Imaging (SWI)
- BLADE
- SPACE
- TimCT Angiography
- TimCT Oncology
- MapIt

Sequence variants

The sequence variants are shown via the parameter card (in the protocol info line) and in the image text. The variant comprises:

- the sequence type (e.g., se for spin echo), and
- the expansions based on the parameters selected

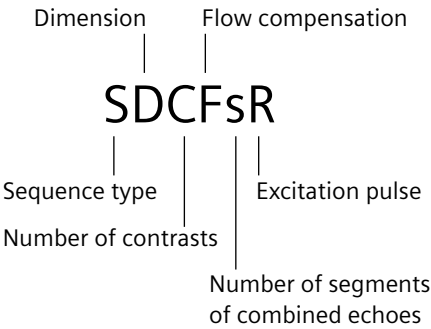

On-screen display

The sequence variants are shown in different ways on-screen.

- In the image text: The *complete* sequence variant is displayed (e.g., fl3d1r_tf)
- In the parameter card: Only the *abbreviation* of the sequence variant is shown (sequence code)

Example: fl_r = FLASH sequence with flow compensation in the readout and slice selection direction.

Displaying the complete sequence variant
Position the mouse pointer on the sequence code.

The sequence variant is shown in full.

Sequence variant components (I)

Sequence type (S)

Abbreviation	Definition
se	Spin echo
ir	Spin echo with inversion recovery
tse	Turbo Spin Echo
tseR	Turbo spin echo with "restore pulse"
tir	Turbo spin echo with inversion recovery
tirR	Turbo spin echo with inversion recovery and "restore pulse"
tgse	Turbo gradient spin echo
tgir	turbo gradient spin echo with inversion recovery
h	HASTE (Half Fourier Single Shot TurboSE)
hir	HASTE with inversion recovery
epfid	EPI-FID
epse	EPI spin echo
epir	EPI spin echo with inversion recovery
fl	FLASH (Fast Low Angle Shot), gradient echo sequence with active RF spoiling
fi	FISP (Fast Imaging with Steady State), Gradient echo sequence without RF spoiling
me	MEDIC (Multi Echo Data Image Combination)
tfl	TurboFLASH
ci	CISS (Constructive Interference in Steady State)
de	DESS (Dual Echo Steady State)
ps	PSIF (time-reversed FISP)

Sequence type (S)

Abbreviation	Definition
spc	SPACE (Sampling Perfection with Application-optimized Contrast using different flip angle Evolutions)
swi	Susceptibility-weighted imaging
tseB	Turbo spin echo with BLADE trajectory
tseBR	Turbo spin echo with BLADE trajectory and "restore pulse"
tirB	Turbo spin echo with inversion recovery and BLADE trajectory
tirBR	Turbo spin echo with inversion recovery, BLADE trajectory and "restore pulse"
re	RESOLVE (REadout Segmentation Of Long Variable Echo trains), multi-shot, diffusion-weighted EPI

Dimension (D)

Abbreviation	Definition
1d	1-dimensional data acquisition
2d	2-dimensional data acquisition
3d	3-dimensional data acquisition

Contrast (C)

Abbreviation	Definition
1, 2, ..., 16, ...	Number of reconstructed images with different contrasts

Sequence variant components (II)

Flow compensation (F)

Abbreviation	Definition
r	Flow compensation in the readout and slice selection direction
rr	Flow compensation in the readout direction only
rs	Flow compensation in the slice direction only
rd	Interleaved acquisition with alternating rephased and dephased measurements.
–	No flow compensation; is displayed only if another character follows
pc	Flow-sensitive gradients for phase-contrast angiography

Number of segments or combined echoes (s)

Abbreviation	Definition
2, 3, ..., 15, ...	Number of segments in the k-space for segmented sequences: $\text{EPI factor} \times \text{Turbo factor} \times \text{segments}$
2, 3, 4, 5, ...	Medic sequences: Number of combined echoes
–	If the number of segments = 1 and the number of combined echoes = 1 (is shown only, if another character follows)

Excitation pulse (R)

Abbreviation	Definition
ns	Non-selective excitation
ts	TONE pulse for slow flow
tm	TONE pulse for moderate flow
tf	TONE pulse for fast flow

Sequence nomenclature (I)

The sequence nomenclature is used in the *syngo* database. It is shown, for example, in the Siemens sequence binder.

Abbreviation	Definition
ciss	Constructive Interference Steady State
dess	Dual Echo Steady State
ep	Echo Planar Imaging
fl	FLASH (fast low angle shot)
gre	Gradient echo sequence
haste	Half Fourier Single Shot Turbo Spin Echo
medic	Multi-Echo Data Image Combination
nav	Sequence with navigator
psif	Time inverted FISP sequence (FISP = fast imaging with steady state precession)
se	Spin echo sequence
tfl	TurboFLASH
tgse	Turbo gradient spin echo
trufi	TrueFISP (FISP = fast imaging with steady state precession)
tse	Turbo spin echo

Abbreviation	Definition
_bold	Sequence for BOLD imaging (BOLD = Blood Oxygen Level Dependency)
_cb	For determining the contrast bolus
_ce	For contrast-enhanced angiography
_ct	For angiography with continuous table move
_diff	Sequence for diffusion contrast
_fid	Free induction decay, e.g., ep_fid: Gradient echo variant of EPI sequence
_field_mapping	For generating a field map for BOLD post-processing
_fq	Flow quantification
_IRT	Sequence for interactive real-time imaging
_mc	Multi-contrast sequence
_pace	Sequence with prospective motion correction
_pc	Phase-contrast angiography
_peri_tof ^a	Time-of-Flight sequence, optimized for peripheral angiography
_r	With flow compensation
_rd ^a	Rephased-dephased angiography sequence
_retro	Sequence with triggered retrospective gating

^a only available at systems with a field strength of 1.5 T

Sequence nomenclature (II)

Abbreviation	Definition
_se	Spin echo sequence, e.g., ep_se: Gradient echo variant of EPI sequence
_seg	Segmented sequence, also refer to ..seg..
_sheco ^a	Shared echo sequence (double contrast TSE)
_shphs	Shared phases sequence
_therm	Temperature-sensitive sequences
_tof	Time-of-Flight (inflow angiography)
_trufi	TrueFISP (FISP = fast imaging with steady state precession), refer to trufi as well
_vibe	Volume interpolated breathhold examination
_vfl	Variable flip angle

^a only available at systems with a field strength of 1.5 T

Abbreviation	Definition
..b..	Bandwidth per pixel; the value follows in Hertz, e.g., se_15b130
..perf..	To measure First Pass perfusion (cardiac imaging)
..r..	With flow compensation, also refer to _r
..seg..	Segmented sequence, also refer to _seg
..ti..	To determine TI (cardiac imaging)
..2d	2D imaging
..3d	3D imaging
.._15..	Echo time, e.g., 15 ms

Application package Tim Application Suite: Spin echo with fixed temporal sequence, sequence description

The Tim Application Suite contains a full set of sequences for clinical routine examinations.

The temporal sequence of the following spin echo sequences is fixed, that is, *independent* of the parameters selected.

Single contrast sequences

Recommendations. The contrast is optimized as a function of TR by varying the flip angle. With a short TR (<500 ms), you can improve T1 contrast by reducing the flip angle to 70 degrees. However, the signal-to-noise ratio is slightly reduced.

se_15b130	Classic spin echo sequence without flow compensation. Use T1 weighting.
se_17rb130^a se_20rb130hf^b	Flow-compensated spin echo sequence. Use Post-gadolinium applications in the head.

^a only available at systems with a field strength of 1.5 T

^b only available at systems with a field strength of 3 T

	se_15b130	se_17rb130^a se_20rb130hf^b
TE variable	✓	–
Contrasts	1	1
Magn. Prep.	IR	IR
Recon. mode	Magnitude/Real ^c	Magnitude/Real ^c
Fat suppression	Fat saturation/ water excitation	Fat saturation
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	✓	✓
Phase Partial Fourier	✓	✓
Averaging mode	Short term/ long term	Short term/ long term
Multi-slice mode	Interleaved/ sequential	Interleaved/ sequential
Flow comp.	No	Yes
Dimension	2D	2D
RF pulse type	Normal	Normal
Gradient mode	Normal	Normal

^a only available at systems with a field strength of 1.5 T

^b only available at systems with a field strength of 3 T

^c may be selected only if Magn.Preparation = IR has been selected

Application package Tim Application Suite: Spin echo with optimized temporal sequence, sequence description

In these sequences, the temporal sequence *depends* on the parameters selected.

se

Spin echo sequence without flow compensation.

Use

As a single contrast sequence, especially well suited for T1-weighted imaging regardless of the body region selected.

Recommendations. Select RF pulse type “Low SAR” to avoid exceeding the SAR limit.

Recommendations. Select blood suppression “On” to reduce pulsation artifacts from blood vessels in T1 weighted brain imaging.

Use

Suitable as a double contrast sequence for orthopedic diagnostics with low readout bandwidth, e.g., shoulders, hips, knees. Dark blood imaging for examining cardiac anatomy by adding dark blood preparation.

se_mc

Multi-contrast sequence with up to 32 contrasts. The sequence design is derived from the TurboSE technique. Since stimulated echoes contribute to the signal with TurboSE, the second echo provides a higher signal contribution than the first echo.

Use

For acquiring T2 relaxation curves.

Recommendations. For T2 image reconstruction, do *not* use the first echo in the calculation.

Application package Tim Application Suite: Spin echo with optimized temporal sequence, parameter ranges

	se	se_mc
TE variable	✓	✓
Contrasts	1–2	1–32
Bandwidth variable	✓	✓
Magn. Prep.	IR	IR
Recon. mode	Magnitude/Real ^a	Magnitude/Real ^a
Fat suppression	Fat saturation/ water excitation/ SPAIR	Fat saturation
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	✓	✓
Phase Partial Fourier	✓	✓
Asymm. Echo	Off/allowed	–
Averaging mode	Short term/ long term	Short term/ long term
Multi-slice mode	Interleaved/ sequential	Interleaved/ sequential
Flow compensation	No	No
Dimension	2D	2D
RF pulse type	Fast/Normal/ Low SAR	Fast/Normal/ Low SAR
Gradient mode	Fast/Normal/ Whisper	Fast/Normal/ Whisper

	se	se_mc
Dark blood	✓	✓
Multi-breathhold	✓	–
2D PACE	Multi-breathhold	–
MapIt	–	✓
Blood suppression	On/off	–

^a may be selected only if Magn.Preparation = IR has been selected

Application package

Tim Application Suite: Turbo spin echo, sequence description (I)

tse

At a turbo factor of 1, the sequence behaves like a spin echo sequence.

Recommendations. If SAR is exceeded, either the flip angle of the refocusing pulse can be reduced and/or RF pulse type “Low SAR” can be selected. A smaller flip angle does not have a noticeable effect on image contrast. As an alternative, the hyperecho technique^a may be used for SAR reduction.

Use

T1/T2 weighting for neuro and ortho imaging with high resolution.

Multislab 3D TurboSE in the neuro area.

Restore technique available.

BLADE technique available.

Evaluation of metastases and lymph nodes in the thorax, abdomen, and pelvis (whole-body imaging with TimCT Oncology).

^a only available at systems with a field strength of 3 T

Recommendations. Slab distance 0, 2 concatenations, 50% oversampling in the slice selection direction. Isotropic resolution is obtained, and any view can be reconstructed using MPR.

Use

Dark fluid neuro imaging.

Recommendations. Select 2 concatenations. This prevents differences in brightness of adjacent slices and suppresses inflow effects from CSF.

Use

Inversion recovery neuro imaging with magnitude or real part image display for pediatric diagnostics.

T2 weighting for breathhold studies in abdominal imaging.

Application package

Tim Application Suite: Turbo spin echo, sequence description (II)

tse
(continued)

Recommendations. High turbo factor, RF pulse type "Fast", high readout bandwidth.

Use

Dark blood imaging for examining cardiac anatomy.

Use

T2 weighting for neuro imaging with Restore technique.

Recommendations. For 3D imaging use a TR >500 ms to obtain good CSF contrast. To prevent loss of signal due to flow phenomena, switch on flow compensation in either the slice selection or readout direction.

Reducing image distortions

MR Conditional implants^a may cause strong off-resonance artifacts. To reduce the artifacts, select the WARP parameter. Use WARP in combination with a high readout bandwidth (approx. 300–500 Hz/Pixel) and a small slice thickness.

^a Please adhere to all safety instructions regarding implants (-> Operator Manual - MR System)

If VAT^b is selected in addition, image distortions can be further reduced. However, VAT may introduce some blurring in the image. To reduce VAT-related blurring, increase the readout bandwidth and reduce the slice thickness. The VAT effect can be scaled from 0% (no VAT) to 100% (full VAT). The appropriate VAT value depends on the level of artifacts and their effect on the anatomic region of interest. In general, a higher level of artifacts requires a higher VAT value.

Do not use conventional spectral fat suppression (including SPAIR) in the presence of strong off-resonance effects, use inversion recovery based fat suppression (STIR) instead.

^b VAT: View Angle Tilting technique, eliminates the signal shift in the frequency-encoding direction caused by off-resonance effects

Application package

Tim Application Suite: Turbo spin echo, sequence description (III)

tse_sheco^a

Shared echo sequence.

Recommendations. If SAR is exceeded, either the flip angle of the refocusing pulse can be reduced and/or RF pulse type “Low SAR” can be selected. A smaller flip angle does not have a noticeable effect on image contrast.

Use

Multi-contrast.

Proton density/T2 double contrast sequence for neuro imaging.

Inversion recovery double contrast imaging with magnitude or real part image display.

^a only available at systems with a field strength of 1.5 T

tse_vfl

3D TurboSE sequence optimized for 3D data acquisition, T1/T2/PD weighting, and dark fluid contrast. Significant SAR reduction through the variable flip angle technique.

Use

SPACE applications.

Display of the entire head with high spatial resolution within an acceptable measurement time.

PD, PD FatSat and T1 weighting with high spatial resolution for orthopedic applications.

tse_contFS

TSE sequence with improved SPAIR fat saturation in free breathing (navigator-triggered) abdominal imaging.

Application package

Tim Application Suite: Turbo spin echo, sequence description (IV)

haste

Single-shot TurboSE sequence.

Use

T2 weighting for neuro applications, used, for example, with uncooperative patients.

T2 weighting for breathhold studies in the abdomen without motion artifacts.

Cholangiography imaging when using very long echo times (~1 s).

Myelography imaging when using very long echo times (~1 s).

Dark blood imaging for examining cardiac anatomy.

Restore technique available.

Evaluation of metastases and lymph nodes in the thorax, abdomen, and pelvis (whole-body imaging with TimCT Oncology).

Recommendations. If SAR is exceeded, either the flip angle of the refocusing pulse can be reduced and/or RF pulse type “Low SAR” can be selected. A smaller flip angle does not have a noticeable effect on image contrast. As an alternative, the hyperecho technique^a may be used for SAR reduction.

^a only available at systems with a field strength of 3 T

Application package

Tim Application Suite: Turbo spin echo,
parameter ranges (I)

	tse	tse_sheco^a
Turbo factor	1–129	5–7
TE variable	✓	✓
Contrasts	1–3	1–2
Bandwidth variable	✓	✓
Magn. Prep.	IR	IR
Recon. mode	Magnitude/Real ^c	Magnitude/Real ^c
Fat suppression	Fat saturation/ SPAIR	Fat saturation
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	✓	✓
Phase Partial Fourier	✓ ^d	✓
Averaging mode	Short term/ long term	Short term/ long term
Multi-slice mode	Interleaved/ sequential	Interleaved/ sequential
Flow compensation	No/Readout/Slice	No/Readout/Slice
Dimension	2D/3D	2D
Elliptical scanning ^b	–	–
Slice resolution ^b	✓	–
Slice Partial Fourier ^b	✓	–
RF pulse type	Fast/Normal/ Low SAR	Fast/Normal/ Low SAR

	tse	tse_sheco^a
Gradient mode	Fast/Normal/ Whisper	Fast/Normal/ Whisper
Dark blood	✓	✓
iPAT	✓	–
Multi-breathhold	✓	–
2D PACE	Multi-breathhold/ Trigger	–
BLADE Trajectory	✓	–
Restore	✓	–
TimCT mode	On/off	–
WARP	✓	–
VAT ^e	0–100%	–

^a only available at systems with a field strength of 1.5 T

^b only if Dimension = 3D is selected

^c may be selected only if Mag. Preparation = IR has been selected

^d parameter cannot be freely set, depends on selected TE

^e only if WARP is selected

Application package

Tim Application Suite: Turbo spin echo, parameter ranges (II)

	tse_vfl	haste
Turbo factor	9–511	1–512 ^d
TE variable	✓	✓
Contrasts	1	1–2
Bandwidth variable	✓	✓
Magn. Prep.	IR/DIR	IR
Recon. mode	Magnitude/Real ^b	Magnitude/Real ^b
Fat suppression	Fat saturation/ SPAIR	Fat saturation/ SPAIR
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	✓	✓
Phase Partial Fourier	✓ ^c	✓ ^c
Averaging mode	Short term	Long term
Multi-slice mode	–	Single-shot
Flow compensation	No/Readout	No
Dimension	3D	2D/3D
Elliptical scanning ^a	–	–
Slice resolution ^a	✓	✓
Slice Partial Fourier ^a	✓	✓
RF pulse type	Fast/Normal/ Optimized	Fast/Normal/ Optimized

	tse_vfl	haste
Gradient mode	Fast/Normal/ Whisper	Fast/Normal/ Whisper
Dark blood	–	✓
iPAT	✓	✓
iPAT ²	✓	–
Multi-breathhold	–	✓
2D PACE	✓	Multi-breathhold/ Trigger
Restore	✓	✓
TimCT mode	–	On/off

^a only if Dimension = 3D is selected

^b may be selected only if Mag. Preparation = IR has been selected

^c parameter cannot be freely set, depends on selected TE

^d parameter cannot be freely set, depends on base and phase resolution

Application package

Tim Application Suite: Gradient echo, sequence description (I)

RF spoiling can be activated with gradient echo sequences. FLASH contrast is generated when RF spoiling is switched on, FISP contrast when RF spoiling is switched off.

gre

Gradient echo sequence

Use

T1 weighting for breathhold studies in abdominal imaging.

Recommendations. Quick parallel sat enables saturation of inflowing blood without significantly increasing measurement time. Quick Fatsat enables fat saturation without significantly increasing measurement time. Water excitation enables fat suppression within acceptable TR increase. Disadvantage: TE is prolonged.

Use

Abdominal imaging In-phase

Opposed-phase in one measurement.

3D FLASH sequence for T1-weighted ortho imaging.

Fast 3D sequence for contrast agent enhancement studies (e.g., dynamic breast diagnostics).

Segmented CINE FLASH sequence, can be combined with line or grid tagging.

Triggered segmented TurboFLASH sequence (activated IR pulse) for “late enhancement” imaging of the myocardium.

Susceptibility-weighted imaging (SWI).

Evaluation of metastases and lymph nodes in the thorax, abdomen, and pelvis (whole-body imaging with TimCT Oncology).

Application package
Tim Application Suite: Gradient echo,
sequence description (II)

FastView Gradient echo sequence

Use
For overview images of large body regions with transverse slices and continuous table move.

Parameter ranges		
	1.5 T	3 T
Matrix	96	96
Slice thickness	5 mm	5 mm
TE/TR	2.19 ms/3.31 ms	1.44 ms/2.56 ms
FoV	480 mm × 87.5%	480 mm × 87.5%
Table speed	36 mm/s	46 mm/s

medic MEDIC sequence (Multi Echo Data Image Combination), gradient echo sequence with flow compensation. When combined echoes = 1, the sequence behaves like a FLASH sequence with flow compensation.

Use
T2*-weighted imaging with a high signal-to-noise ratio for the spine (especially transverse cervical and thoracic spine) and ortho (knee and shoulder) imaging.
T2*-weighted 3D imaging of the cervical spine with a small flip angle and adjusted TR.

tfl

Single-shot TurboFLASH sequence.

Use

3D tfl for fast T1-weighted volume measurements of the head.

2D tfl with dark blood preparation for low resolution imaging of the cardiac anatomy.

2D tfl combined with saturation recovery preparation for contrast agent enhancement studies.

2D tfl to determine the transit time of a test bolus as preparation for CE angiography.

Recommendations. To prevent saturation effects, use the "long term" averaging mode. All slices will then be measured sequentially for one averaging, before the next averaging measures the series of slices again.

Application package

Tim Application Suite: Gradient echo, parameter ranges (I)

	gre
Segments	1–127
Combined echoes	–
TE variable	✓
Contrasts	1–12
Bandwidth variable	✓
Magn. Prep.	IR, SR ^a
Reconstruction mode	Magnitude/Phase
Fat suppression	Fat saturation/ water excitation
Saturation regions	Regular/Parallel/Tracking
MTC	✓
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Interleaved/sequential
Flow compensation	Yes/No/Readout/Slice/ Slice&Readout
Dimension	2D/3D
Elliptical scanning ^b	✓
Slice resolution ^b	✓

	gre
Slice Partial Fourier ^b	✓
Excitation pulses ^b	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	On/off
Gradient mode	Fast/Normal/Whisper
Dark blood	✓ ^a
Grid/line tagging	✓
iPAT	✓
iPAT ²	✓
Multi-breathhold	✓
2D PACE	Multi-breathhold
Readout mode	Monopolar/Bipolar
SWI	✓
PACE	✓
MapIt	✓
TimCT mode	On ^d /off

^a if segments >1 (segmented TurboFLASH)

^b only if Dimension = 3D is selected

^c may be selected only if Mag. Preparation = IR has been selected

^d when switched on, DIXON reconstruction can be selected

Application package

Tim Application Suite: Gradient echo, parameter ranges (II)

	medic	tfl
Segments	–	–
Combined echoes	1 – 12	–
TE variable	✓	Min.
Contrasts	1	1
Bandwidth variable	✓	✓
Magn. Prep.	–	IR, SR
Recon. mode	Magnitude	Magnitude/Real ^c
Fat suppression	Fat saturation/ water excitation	Water excitation
Saturation regions	Regular/Parallel	–
MTC	✓	–
Phase Partial Fourier	✓	✓
Asymm. Echo	–	✓
Averaging mode	Short term/ long term	Long term
Multi-slice mode	Interleaved/ sequential	Single-shot
Flow compensation	Yes	No
Dimension	2D/3D	2D/3D
Elliptical scanning ^b	✓	–
Slice resolution ^b	✓	✓

	medic	tfl
Slice Partial Fourier ^b	✓	✓
Excitation pulses ^b	Slab-selective	Slab-selective/ non-selective
RF pulse type	Fast/Normal	Fast/Normal
RF spoiling	On/off	Off
Gradient mode	Fast/Normal/ Whisper	Fast/Normal/ Whisper
Dark blood	–	✓
Grid/line tagging	–	–
iPAT	✓	✓
iPAT ²	–	–
Multi-breathhold	–	✓
2D PACE	–	Multi-breathhold/ Trigger

^a if segments >1 (segmented TurboFLASH)

^b only if Dimension = 3D is selected

^c may be selected only if Mag. Preparation = IR has been selected

^d only if Dimension = 2D is selected

Application package Tim Application Suite: Steady-state gradient echo, sequence description

With steady-state sequences, echo times TE and repetition times TR are set to fixed minimum values to provide an optimal image quality. In case of the psif sequence, this applies to TE only, TR is a freely-adjustable parameter.

psif

Gradient echo sequence with flow compensation in slice or readout direction, but highly sensitive to motion artifacts. At a large flip angle, strongly T2-weighted images.

Use

T2-weighted imaging with 3D PSIF with flow compensation in readout direction, for CSF or spine diagnostics.

T2-weighted imaging with 2D or 3D PSIF with flow compensation in slice selection direction, for breathhold studies of the abdomen: Dark blood T2 weighting in the liver.

	psif
TE variable	Min.
Contrasts	1
Bandwidth variable	✓
Recon. mode	Magnitude
Fat suppression	Water excitation
Phase Partial Fourier	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Readout/slice
Dimension	2D/3D
Elliptical scanning ^a	✓
Slice resolution ^a	✓
Slice Partial Fourier ^a	✓
Excitation pulses ^a	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
iPAT	✓
Diffusion weighting	Yes

^a only if Dimension = 3D is selected

Application package Tim Application Suite: Gradient echo for inflow angiography (ToF), sequence description

fl_tof	FLASH sequence. Use Inflow angiography with 2D or 3D acquisition. 3D display of intracranial vessels in sequential slice acquisition. Display of the coronary arteries using 3D technique in sequential slice acquisition. Application for 2D Time-of-Flight examinations. Recommendations. For 3 dimensional applications, select the TONE pulse (depending on flow velocity) to counteract the saturation effect of blood flowing through the slab.
---------------	--

	fl_tof
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Recon. mode	Magnitude
Saturation regions	Regular/Parallel/Tracking
MTC	✓
Phase Partial Fourier	✓
Asymm. Echo	Allowed
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	2D/3D
Elliptical scanning ^b	✓
Slice resolution ^b	✓
Slice Partial Fourier ^b	✓
Excitation pulse	Slab-selective
RF pulse type	Normal ^a
RF spoiling	On
Gradient mode	Fast/Normal/Whisper
iPAT	✓

^a the TONE pulse can be selected via the flow velocity parameter, optimized for slow, moderate, or fast flow

^b only if Dimension = 3D is selected

Application package Tim Application Suite: Contrast-enhanced angiography, sequence description

tfl_cb	2D single-shot TurboFLASH sequence. Use Optimized for determining arrival of bolus as preparation for contrast-enhanced angiography.
fl3d_ce	Gradient echo sequence Use Optimized for CE angiography. Angiography of the carotid arteries. Angiography of the thoracic arteries. Angiography of the pulmonary arteries. Table stepping angiography for display of peripheral vessels. Cardiac imaging to examine “Myocardial Viability” with triggered segmented 3D FLASH sequence with activated IR pulse. Recommendations. For suppressing background signal, select fat suppression (fat saturation or water excitation). Recommendations. For CARE examinations, select “3D centr. reordering” on the Angio parameter card.

Recommendations. Set inversion time TI so that the signal from the healthy myocardium is at a minimum.

Use

Cardiac imaging to examine the coronary arteries with a triggered segmented 3D FLASH sequence with fat suppression.

Recommendations. An IR pulse can be used instead of the fat suppression pulse. In this case, set the inversion time to suppress fat.

fl3d_vibe

Gradient echo sequence

Use

For contrast-enhanced examinations of the upper abdomen.

Recommendations. For suppressing background signal, select fat suppression (fat saturation or water excitation).

Application package Tim Application Suite: Contrast-enhanced angiography, parameter ranges (I)

	tfl_cb
Segments	–
TE variable	Min.
Contrasts	1
Bandwidth variable	✓
Magn. Prep.	IR/SR
Recon. mode	Magnitude/Real ^c
Fat suppression	Water excitation
Saturation regions	–
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	Off/allowed
Averaging mode	Long term
Multi-slice mode	Single-shot
Flow compensation	No

	tfl_cb
Dimension	2D
Elliptical scanning ^d	–
Slice resolution ^d	–
Slice Partial Fourier ^d	–
Excitation pulse	Slice-selective
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal
Dark blood	✓
CARE Bolus	–
iPAT	–
iPAT ²	–
Multi-breathhold	–
2D PACE	–

^a if segments >1 (segmented TurboFLASH)

^b Partial Fourier is selected. However, the setting cannot be changed

^c may be selected only if Magn. Preparation = IR or SR has been selected

^d only if Dimension = 3D is selected

Application package Tim Application Suite: Contrast-enhanced angiography, parameter ranges (II)

	fl3d_ce	fl3d_vibe
Segments	1–127	–
TE variable	Min.	✓ ^e
Contrasts	1	1–2
Bandwidth variable	✓	✓
Magn. Prep.	IR ^a	–
Recon. mode	Magnitude	Magnitude
Fat suppression	Fat saturation/ water excitation	Fat saturation/ water excitation/ SPAIR
Dixon	–	✓
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	–	–
Phase Partial Fourier	✓ ^b	✓
Asymm. Echo	Allowed	Off/allowed
Averaging mode	Short term	Short term
Multi-slice mode	Interleaved/ sequential	Interleaved/ sequential
Flow compensation	No	No

	fl3d_ce	fl3d_vibe
Dimension	2D/3D	3D
Elliptical scanning ^d	✓	✓
Slice resolution ^d	✓	✓
Slice Partial Fourier ^d	✓ ^b	✓ ^b
Excitation pulse	Slab-selective	Slab-selective
RF pulse type	Fast/Normal	Fast/Normal
RF spoiling	On	On
Gradient mode	Fast/Normal	Fast/Normal
Dark blood	–	–
CARE Bolus	✓	✓
iPAT	✓	✓
iPAT ²	✓	✓
Multi-breathhold	–	✓
2D PACE	–	Multi-breathhold
Readout mode	–	Monopolar/Bipolar
Liver registration	–	✓
MapIt	–	✓

^a if segments >1 (segmented TurboFLASH)

^b Partial Fourier is selected. However, the setting cannot be changed

^c may be selected only if Magn. Preparation = IR or SR has been selected

^d only if Dimension = 3D is selected

^e The sequence allows a freely-selectable TE, an automatic minimal TE, or an automatic TE set to the “in-phase” or “opposed-phase” time

Application package Tim Application Suite: Rephased-dephased angiography, sequence description

fl3d_rd^a

Magnitude contrast gradient echo sequence.

Use

To display the arteries of the leg with a 3D measurement.

^a only available at systems with a field strength of 1.5 T

	fl3d_rd^a
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Reconstruction mode	Magnitude
Fat suppression	Fat saturation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	3D
Elliptical scanning	✓
Slice resolution	✓
Slice Partial Fourier	✓
Excitation pulse	Slab-selective
RF pulse type	Normal
RF spoiling	On
Gradient mode	Fast/Normal/Whisper

^a only available at systems with a field strength of 1.5 T

Application package Tim Application Suite: Inflow angiography (ToF), sequence description

fl_peri_tof^a

2D FLASH sequence.

Use

Peripheral angiography.

ECG-triggered measurement of vessels in the legs at a high heart rate or in the kidneys, arms, and carotid arteries.

Recommendations. Perform data acquisition during the systole to obtain the maximum signal and avoid pulsation artifacts.

^a only available at systems with a field strength of 1.5 T

	fl_peri_tof ^a
Segments	1 – 23
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	Regular/Parallel/Tracking
MTC	✓
Phase Partial Fourier	✓
Asymm. Echo	Off/allowed
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	2D
Excitation pulse	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal/Whisper

^a only available at systems with a field strength of 1.5 T

Application package Tim Application Suite: Phase-contrast angiography, sequence description

fl_pc

FLASH sequence. Possible online reconstructions: magnitude image, phase image, magnitude sum image.

Use 2D

Peripheral angiography, e.g., for acquiring large fluctuations in flow velocity (Multi-venec application). Also as a localizer for 3D phase contrast measurements.

Use 3D

Neuro applications, e.g., to display arterial vessel systems.

You can set the following established applications on the "Angio" parameter card:

- Multi-venec applications:
variable velocity encoding in one spatial direction
- Single-venec applications:
Same velocity encoding in 3 spatial directions
- Mixed venec applications:
free selection of direction and velocity for 3 encodings

	fl_pc
Segments	1 – 25
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Reconstruction mode	Magnitude
Saturation regions	Regular/Parallel/Tracking
MTC	✓
Phase Partial Fourier	–
Asymm. Echo	✓
Averaging mode	Off/Weak/Strong
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	2D/3D
Elliptical scanning ^a	✓
Slice resolution ^a	✓
Slice Partial Fourier ^a	–
Excitation pulse	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal/Whisper
Venc cm/s	1 – 999

^a only if Dimension = 3D is selected

Application package Tim Application Suite: Fast dynamic imaging, sequence description

TWIST

Gradient echo sequence. Faster sequences of 3D image data than with a standard gradient echo sequence.

Use

To evaluate dynamic processes with high spatial and temporal resolution.

Recommendations. In the **Angio/Common** parameter card: The parameter **Central region A** provides the size of the central k-space and the parameter **Sampling density B** indicates the sampling density in the peripheral region. To increase temporal resolution, either reduce parameter A or B.

TE variable	Min.
Contrasts	1
Bandwidth variable	✓
Reconstruction mode	Magnitude
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	Off/Weak/Strong
Averaging mode	Short term
Multi-slice mode	Interleaved/sequential
Flow compensation	No
Dimension	3D
Elliptical scanning	✓
Slice resolution	✓
Slice Partial Fourier	✓
Excitation pulses	Slab-selective
RF pulse type	Fast/Normal/Low SAR
RF spoiling	On
Gradient mode	Fast/Normal
iPAT	✓
iPAT ²	✓
Central region A	4–100%
Sampling density B	0–50%
Temporal interpolation	✓
Time stamp in image	✓

Application package Tim Application Suite: TrueFISP, sequence description (I)

truFi

TrueFISP steady-state gradient echo sequence.

Recommendations. Minimize TR by selecting a high readout bandwidth to avoid interference streaks in the image.

Use

T2 weighting for neuro applications, used, for example, with uncooperative patients. T2 weighting for breathhold studies in the abdomen without motion artifacts.

TE variable	Min.
Contrasts	1
Bandwidth variable	✓
Magn. Prep.	IR, SR
Reconstruction mode	Magnitude
Fat suppression	Fat saturation/ water excitation
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	No ^a
Dimension	2D/3D
Elliptical scanning ^b	✓
Slice resolution ^b	✓
Slice Partial Fourier ^b	✓
Excitation pulses ^b	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
iPAT	✓
iPAT ²	✓
Multi-breathhold	✓
2D PACE	Multi-breathhold

^a TrueFISP is essentially flow-compensated from one RF pulse to the next

^b only if Dimension = 3D is selected

Application package Tim Application Suite: TrueFISP, sequence description (II)

CV (without ECG)

Sequence type	Cine	Define	Shots per slice	View sharing
Trufi	On	Shots	1	Shared phases

Fast single-shot TrueFISP sequence with phase sharing. Measurement and reconstruction of multiple images (phases) in a single cardiac cycle.

Use

For displaying dynamic processes.
To display cardiac motion without a breath-hold phase.
To examine cardiac volume in a breathhold phase; multi-phase measurement of multiple sequential slices is possible.

Please note: The sequence can run without triggering for real-time monitoring of cardiac or other motions. If only the Tim Application Suite is available, ECG/pulse triggering is not available.

TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Prep.	–
Reconstruction mode	Magnitude
Fat suppression	–
Phase Partial Fourier	–
Asymm. Echo	Possible
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^b
Dimension	2D
Elliptical scanning ^c	–
Slice resolution ^c	–
Slice Partial Fourier ^c	–
Excitation pulses ^c	–
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
iPAT	✓
iPAT ²	–
Multi-breathhold	–
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b TrueFISP is essentially flow-compensated from one RF pulse to the next

^c only if Dimension = 3D is selected

Application package Tim Application Suite: TrueFISP, sequence description (III)

CV (without ECG)

Sequence type	Define	Shots per slice	Magn. preparation
Trufi	Shots	1	IR/SR/SR perf

Single-shot TrueFISP sequence.
Can be combined with inversion recovery and saturation recovery preparation pulses. Image reconstruction allows for Partial Fourier factors of 4/8 and 5/8.

Saturation Recovery (SR) or Saturation Recovery Perfusion (SR perf)?

- SR: Rectangular saturation pulse (normally 90 degrees)
- SR perf: Echo train with 3 saturation pulses (90 degrees each) as well as different time intervals and gradient spoilers. More robust with respect to magnetic field inhomogeneities, however, with a higher SAR.

Use

To measure First Pass perfusion.
For sequential multi-slice applications.

Segments	Variable ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	IR, SR, selective, non-selective
Reconstruction mode	Magnitude
Fat suppression	Possible
Saturation regions	–
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^c
Dimension	2D/3D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	–
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Tim Application Suite: TrueFISP, sequence description (IV)

CV

Sequence type	Cine
Trufi	On

Segmented TrueFISP sequence.
The sequence is triggered prospectively.
The sequence runs continuously to maintain the steady state.

Use

To display cardiac motion. Provides good contrast of blood and myocardium.

Segments	3–31
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No
Dimension	2D (only untriggered)
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	✓
2D PACE	Multi-breathhold

^a TE is automatically set to the minimum and cannot be changed

Application package Tim Application Suite: TrueFISP, sequence description (V)

CV

Sequence type	Cine
Trufi	Off

Segmented TrueFISP sequence.
It can be combined with a variety of selective or non-selective preparation pulses (fat saturation, inversion recovery, saturation recovery, and dark blood).

Use

For 2D or 3D applications.
To characterize tissue and angiography.

Segments	Variable ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	IR, SR, selective, non-selective
Reconstruction mode	Magnitude
Fat suppression	✓
Saturation regions	Regular/Parallel
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^c
Dimension	2D/3D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	✓
Tagging	–
iPAT	✓
Multi-breathhold	✓
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Tim Application Suite: TrueFISP, sequence description (VI)

CV

Sequence type	Cine	Magn. preparation
Trufi	On	T1 Scout

TrueFISP sequence. After a single preparation pulse, several images can be acquired—either segmented or with the single-shot technique. The contrast of result images varies depending on the time duration TI following the preparation pulse.

Use

For T1 mapping and determining a suitable TI.

Segments	Variable ^a
TE variable	–
Contrasts	Variable
Bandwidth variable	✓
Magn. Preparation	TI Scout
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	–
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	–
Multi-breathhold	–
2D PACE	–

^a max. number of segments depends on the number of lines

Application package Tim Application Suite: TrueFISP, sequence description (VII)

trufi_ freqScout

TrueFISP sequences. Several images of identical geometry, but different offset frequency are acquired. The distance of the frequency shifts and the number of images are controlled via the parameters **TruFi delta freq.** and **Measurements**. The offset frequencies are included in the image text. A visual analysis in the Viewer determines the optimal frequency. It is entered in subsequent measurements for the **TruFi delta freq.** parameter.

Use

Especially with TrueFISP protocols it may be necessary to adjust the offset frequency based on the image to move the typical TrueFISP stripe artifacts out of the region of interest.

Segments	Variable
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential/ Single measurement
Flow compensation	–
Dimension	2D
RF pulse type	Fast/Normal/Low SAR
RF spoiling	–
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	–
2D PACE	–

Application package Tim Application Suite: EPI sequences, sequence description

ep2d_se	Single-shot spin echo EPI sequence. Use To examine T2-weighted lesions. Recommendations. By activating an inversion pulse with a long inversion time, the CSF signal in the head can be suppressed.
ep_seg_fid	Segmented FID EPI sequence. Faster than gradient echo sequences, less off resonance effects than the single-shot FID EPI sequence. Use T2*-weighted 2D/3D imaging in the head.

ep_seg_se

Segmented spin echo EPI sequence. Faster than spin echo sequences, less off resonance effects than a single-shot spin echo EPI sequence.

Use

Fast T2-weighted 2D/3D imaging in the head.

Application package Tim Application Suite: EPI sequences, parameter ranges

	ep2d_se
EPI Factor	1–256 ^a
TE variable	✓
Contrasts	1
Bandwidth variable	Min ... max
Magn. Preparation	IR
Recon. mode	Magnitude
Fat suppression	Fat saturation/ water excitation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Averaging mode	Long term
Multi-slice mode	Single-shot
Flow compensation	No
Dimension	2D
RF pulse type	Normal
RF spoiling	Off
Gradient mode	Fast
iPAT	✓
Multi-breathhold	–
2D PACE	–

ep_seg_fid	ep_seg_se
1 – 127	1 – 127
✓	✓
1	1
Min ... max	Min ... max
–	IR
Magnitude	Magnitude
Fat saturation/ water excitation	Fat saturation/ water excitation
Regular/Parallel	Regular/Parallel
✓	✓
✓	✓
Long term	Long term
Interleaved/ sequential	Interleaved/ sequential
No	No
2D/3D	2D/3D
Normal	Normal
On/Off	Off
Fast/Normal	Fast/Normal
–	–
✓	✓
Multi-breathhold	Multi-breathhold

^a parameter cannot be freely set, depends on base and phase resolution

Application package CISS & DESS: Sequence description

The CISS & DESS package includes special 3D sequences.

dess

3D gradient echo sequence

Use

Primarily in orthopedic imaging with good contrast between synovial fluid and cartilage.

Recommendations. A non-selective excitation pulse is activated beforehand for fat suppression at a short TR.

ciss

3D gradient echo sequence for T2 imaging at a large flip angle. TE and TR are permanently set to a minimum value to provide an optimal image quality.

Use

Can be used in neurology, where CSF provides contrast: cochlea, labyrinth, cranial nerves, optic nerve tract, spinal canal, etc.

	dess	ciss
TE variable	✓	Min.
Contrasts	1	1
Bandwidth variable	✓	✓
Recon. mode	Magnitude	Magnitude
Fat suppression	Water excitation	Water excitation
Phase Partial Fourier	✓	✓
Averaging mode	Short term/ long term	Short term
Multi-slice mode	Sequential	Sequential
Flow compensation	Readout	No
Dimension	3D	2D/3D
Elliptical scanning ^a	✓	✓
Slice resolution ^a	✓	✓
Slice Partial Fourier ^a	✓	✓
Excitation pulses ^a	Slab-selective/ non-selective	Slab-selective
RF pulse type	Fast/Normal	Fast/Normal
RF spoiling	Off	Off
Gradient mode	Fast/Normal/ Whisper	Fast/Normal/ Whisper
iPAT	✓	–

^a only if Dimension = 3D is selected

Application package TGSE: Sequence description

The TGSE package contains an ultrafast turbo gradient spin echo sequence for high resolution imaging or extremely short measurement times.

tgse

At an EPI factor of 1 and a Turbo factor > 1 , the sequence behaves like a tse sequence. At a Turbo factor of 1 and an EPI factor > 1 , the sequence behaves like a segmented EPI sequence.

Recommendations. If SAR is exceeded, either the flip angle of the refocusing pulse can be reduced and/or RF pulse type "Low SAR" can be selected. A smaller flip angle does not have a noticeable effect on image contrast.

Use

T2 weighting for high-resolution neuro or ortho imaging in an acceptable measurement time (recommended EPI factor at a high turbo factor ≤ 3).

Inversion recovery neuro imaging with magnitude or real value image display.

Please note: Increasing the EPI factor increases the sequence's susceptibility sensitivity; distortion artifacts may increase.

Application package TGSE: Parameter ranges

	tgse
Turbo factor	1–65
EPI factor	1–21
TE variable	✓ ^b
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	IR
Reconstruction mode	Magnitude/Real ^a
Fat suppression	Fat saturation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	–
Averaging mode	Short term/long term
Multi-slice mode	Interleaved/sequential
Flow compensation	No
Dimension	2D
RF pulse type	Fast/Normal/Low SAR
Gradient mode	Fast/Normal/Whisper
Dark blood	✓
Multi-breathhold	✓
2D PACE	Multi-breathhold

^a may be selected only if Magn.Preparation = IR has been selected

^b applies only, when turbo factor = 1

Application package AutoAlign: Sequence description

AALScout

Modified fl3d_vibe sequence for AutoAlign scouts in AutoAlign programs. For adjusting, measuring 3D volumes, and computing AutoAlign matrices.

The algorithm uses bone markers (L = landmark-based) for automatic slice positioning.

Use

The sequence must precede any examination with AutoAlign. The slice position of subsequent measurement protocols is automatically adjusted with AutoAlign.

Please note: The sequence parameters cannot be changed. *Exception:* coil selection and iPAT factor.

Application package Advanced Cardiac:
Sequence description (I)

The CV sequence combines a multitude of functions which were implemented in various cardio sequences in previous software versions. These include, e.g., functions such as retrospective triggering, radial k-space sampling, shared phases, GRE and TrueFISP contrast, 2D/3D acquisitions, magnetization preparations, Cine, TI Scout, etc..

CV

Sequence type	Cine	1st Signal/Mode
Trufi	On	ECG/Retro

Segmented TrueFISP sequence. Triggered, retrospective gating: Measurement of the k-space lines is triggered prospectively, however, the measurement data are sorted and reconstructed retrospectively. As a result, the entire cardiac cycle can be acquired.

Use

To display cardiac motion of a complete cardiac cycle. Provides good contrast of the blood and myocardium. Particularly suited for patients with arrhythmias.

Segments	Variable ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	✓
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

Application package Advanced Cardiac:
Sequence description (II)

CV

Sequence type	Cine	View sharing	1st Signal/ Mode
Trufi	On	Shared phases	ECG/Trigger

Similar to the previous sequence, however, with phase sharing for improved temporal resolution.

Use

To display cardiac motion. Provides good contrast of blood and myocardium.
For short breathhold studies or multiple slice measurements within one breathhold phase.

Segments	Variable ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^c
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	✓
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Advanced Cardiac:
Sequence description (III)

CV

Sequence type	Cine	Trajectory
Trufi	On	Radial

Segmented TrueFISP sequence.
The sequence is triggered prospectively or retrospectively. Radial sampling of the k-space improves temporal and spatial resolution.

Use
To display cardiac motion.

Segments	Variable ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	–
Multi-breathhold	✓
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

Application package Advanced Cardiac:
Sequence description (IV)

CV

Sequence type	Cine	1st Signal/Mode
Gre	On	ECG/Retro

Segmented FLASH sequence. Triggered retrospective gating possible.

Use

To display cardiac motion. Especially well suited for the display of cardiac valve diseases. In particular for patients with arrhythmias.

Segments	–
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	Regular/Parallel
MTC	–
Phase Partial Fourier	–
Asymm. Echo	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	Yes/No/Slice&Readout
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	✓
iPAT	✓
Multi-breathhold	✓
2D PACE	–

Application package Advanced Cardiac:
Sequence description (V)

CV

Sequence type	Cine	1st Signal/ Mode	View sharing
Gre	On	ECG/Trigger	Shared phases

2D shared phase gradient echo sequence.

Use

To display cardiac motion.

Segments	Variable ^a
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	Fat saturation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes/No/Slice&Readout
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	On/off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	✓
iPAT	–
Multi-breathhold	✓
2D PACE	Multi-breathhold

^a max. number of segments depends on the number of lines

Application package Advanced Cardiac:
Sequence description (VI)

CV (with ECG)

Sequence type	Cine	Define	Shots per slice	View sharing	1st Sig- nal/ Mode
Trufi	On	Shots	1	Shared phases	ECG/ Trigger

Fast single-shot TrueFISP sequence with phase sharing. Measurement and reconstruction of multiple images (phases) in a single cardiac cycle.

Use

To display cardiac motion without a breath-hold phase. To examine cardiac volume in a breathhold phase; multi-phase measurement of multiple sequential slices is possible.

Please note: The sequence can be run without triggering for real-time monitoring of cardiac or other motions.

Segments	–
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^b
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	✓
Multi-breathhold	–
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

^b TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Advanced Cardiac:
Sequence description (VII)

CV

Sequence type	Cine	Trajectory	Define	Shots per slice
Trufi	On	Radial	Shots	1

Real-time TrueFISP sequence to measure multiple images in a cardiac cycle; with or without ECG synchronization. Radial sampling of the k-space improves temporal and spatial resolution.

Use

To display cardiac motion in real time.

Segments	–
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	–
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	–
iPAT	–
Multi-breathhold	✓
2D PACE	–

^a TE is automatically set to the minimum and cannot be changed

Application package Advanced Cardiac: Sequence description (VIII)

CV_nav	Combination of CV sequence (sequence type Trufi, Cine Off) and the prospective measurement of a navigator echo. Use To display the coronary arteries with free breathing.
fl3d_ce_nav	Combination of the fl3d_ce sequence and the prospective measurement of a navigator echo. Use To display the coronary arteries with free breathing.
tse_nav	2D TurboSE with dark blood preparation and the prospective measurement of a navigator echo. Use To display the morphology of the heart and coronary arteries with free breathing.

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

	CV_nav	fl3d_ce_nav	tse_nav
Segments	Variable ^b	Variable ^b	–
TE variable	– ^a	✓	✓
Contrasts	1	1	1
Bandwidth variable	✓	✓	✓
Magn. Preparation	IR, SR, selective, non-selective	IR, selective, non-selective	–
Recon. mode	Magnitude	Magnitude	Magnitude
Fat suppression	✓	✓	✓
Saturation regions	Regular/Parallel	Regular/Parallel	Regular/Parallel
Phase Partial Fourier	✓	✓	–
Asymm. Echo	✓	3 (fixed)	–
Averaging mode	Short term	Short term	Short term
Multi-slice mode	Sequential	Sequential	Interleaved
Flow compensation	No ^c	Yes	No
Dimension	2D/3D	3D	2D/3D
RF pulse type	Fast/Normal	Fast/Normal	Fast/Normal
RF spoiling	Off	Off	Off
Gradient mode	Fast/Norm./Whisp.	Fast/Norm./Whisp.	Fast/Norm./Whisp.
Dark blood	✓	–	✓
iPAT	✓	✓	–

Application package Advanced Cardiac:
Sequence description (IX)

CV

Sequence type	Cine	Flip angle mode
Gre	Off	Variable

2D gradient echo sequence with a variable flip angle.

Use

Display of individual slices within a breath-hold phase.

Recommendations. To increase signal intensity, each line is measured at a different flip angle. Since the magnetization is saturated, it is necessary to wait for the next cardiac cycle to allow for recovery of the magnetization. Therefore, only one cardiac phase can be measured.

Segments	1–23
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	Fat saturation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	On/off
Gradient mode	Fast/Normal/Whisper
Dark blood	–
Tagging	✓
iPAT	–
Multi-breathhold	✓
2D PACE	Multi-breathhold

Application package Advanced Cardiac:
Sequence description (X)

CV (with ECG)

Sequence type	Define	Shots per slice	Magn. prepara- tion	1st Sig- nal/Mode
Trufi Gre Gre epi	Shots	1	IR/SR/SR perf	ECG/Trig- ger

Single-shot sequences. Can be combined with inversion recovery or saturation recovery preparation pulses. Image reconstruction allows for Partial Fourier factors of 6/8 and 7/8 (Trufi and Gre).

Saturation Recovery (SR) or Saturation Recovery Perfusion (SR perf)?

- SR: Rectangular saturation pulse (normally 90 degrees)
- SR perf: Echo train with 3 saturation pulses (90 degrees each) as well as different time intervals and gradient spoilers. More robust with respect to magnetic field inhomogeneities, however, with a higher SAR.

Use

To measure First Pass perfusion.
For sequential multi-slice applications.

Segments	Fixed ^b
TE variable	— ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	IR, SR, selective, non-selective
Reconstruction mode	Magnitude
Fat suppression	Yes (Gre epi)
Saturation regions	—
MTC	—
Phase Partial Fourier	—
Asymm. Echo	✓
Averaging mode	Long term
Multi-slice mode	Single-shot
Flow compensation	No ^c (Gre)
Dimension	2D/3D
RF pulse type	Fast/Normal
RF spoiling	On (Gre and Gre epi)
Gradient mode	Fast/Normal/Whisper
PAT	Integrated/tPAT

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Advanced Cardiac:
Sequence description (XI)

CV (with ECG)

Sequence type	Magn. preparation	1st Signal/ Mode	Recon- struction
Trufi Gre	IR	ECG/Trigger	Magnitude/ Real

TrueFISP and TurboFLASH sequences (segmented and single-shot) to create phase-sensitive inversion recovery images (real part and magnitude images). The contrast in real part images is less dependent on the optimal selection of the inversion time. Image reconstruction allows for Partial Fourier factors of 6/8 and 7/8 (Trufi and Gre).

Use

To display late enhancement.

Segments	Variable and fixed ^b
TE variable	– ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	IR, selective, non-selective
Reconstruction mode	Magnitude/Real
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	–
Asymm. Echo	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No ^c (Gre)
Dimension	2D
RF pulse type	Fast/Normal
RF spoiling	On (Gre)
Gradient mode	Fast/Normal/Whisper
PAT	Integrated

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines
(variable = segmented, fixed = single-shot)

^c TrueFISP is essentially flow-compensated from one RF pulse to the next

Application package Flow Quantification: Sequence description

The Flow Quantification package contains sequences for quantitative flow measurements.

fl_fq Segmented FLASH sequence with variable flow encoding. The sequence measures one flow-compensated and one flow-encoded measurement. Possible online reconstructions: Magnitude image, phase image, magnitude sum image

Use

To display and quantify blood flow. Through-plane measurements for flow quantification and in-plane measurements for flow display.

fl_fq_retro Segmented FLASH sequence with variable flow encoding. The sequence measures one flow-compensated and one flow-encoded measurement. Possible online reconstructions: Magnitude image, phase image, magnitude sum image. Triggered, retrospective gating possible.

Use

To display and quantify blood flow during complete heart cycle coverage. Particularly suited for patients with arrhythmias.

fl_fq_shphs

Segmented FLASH sequence with phase sharing and variable flow encoding. The sequence measures a flow-compensated and a flow-encoded scan. Phase sharing enables more frequent sampling of the center raw data lines during pulsating flow.

Use

To display and quantify blood flow.

Through-plane measurements for flow quantification and in-plane measurements for flow display. Enables flow measurement in breathhold technique using phase sharing.

Application package Flow Quantification: Parameter ranges

	fl_fq
Segments	1–25
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Recon. mode	Magnitude
Saturation regions	Regular/Parallel/Tracking
MTC	✓
Phase Partial Fourier	–
Asymm. Echo	✓
Averaging mode	Short term/long term
Multi-slice mode	Sequential
Flow compensation	Yes
Dimension	2D
Excitation pulse	Slice-selective
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal/Whisper
Venc cm/s	2–999
Multi-breathhold	–

^a TE is automatically set to the minimum and cannot be changed

^b max. number of segments depends on the number of lines

fl_fq_retro	fl_fq_shphs
Variable ^b	3–7
– ^a	✓
1	1
✓	✓
Magnitude	Magnitude
Regular/Parallel	Regular/Parallel
–	–
–	–
–	3 (fixed)
Short term	–
Sequential	Sequential
Yes	Yes
2D	2D
Slice-selective	Slice-selective
Fast/Normal	Fast/Normal
On	On
Fast/Normal/Whisper	Fast/Normal/Whisper
2–999	2–999
✓	–

Diffusion Imaging: Sequence description

Prerequisites: Inline Diffusion and Advanced Functional Neuro. The basic functionality is already included in the Tim Application Suite.

ep2d_diff

Single-shot spin echo EPI sequence.

Use

For diffusion imaging, e.g., for examining strokes.

Recommendations. To minimize image distortions through susceptibility, select a bandwidth that enables use of minimum echo spacing.

Note. Diffusion-specific parameters are selected from the Diff parameter card: Direction(s) of the diffusion-sensitive axis(es) (diffusion mode), number and magnitude of b-values, reconstruction mode (ADC image, Trace images).

resolve

Multi-shot, diffusion-weighted, readout-segmented EPI sequence.

During diffusion preparation, multi-shot DWI is sensitive to brain motion caused by CSF pulsation. This leads to non-linear phase errors that vary from shot to shot. The effect of these phase errors can be minimized by using a readout-segmented EPI readout in conjunction with 2D navigator phase correction and navigator-based reacquisition.

Use

For improved image quality in neuro imaging compared to standard single-shot EPI sequence.

Recommendations. For a given spatial resolution, reduce the minimum echo spacing (and the associated artifacts) by increasing the number of "Readout segments". For a fixed echo spacing, increase the available spatial resolution by increasing the number of "Readout segments".

Diffusion imaging: Parameter ranges

	ep2d_diff	resolve
EPI Factor ^a	1 – 256	1 – 256
TE variable	✓	– ^b
Contrasts	1	2
Bandwidth variable	Min ... max	– ^b
Magn. Preparation	IR	IR
Recon. mode	Magnitude	Magnitude
Fat suppression	Fat saturation/ water excitation/ SPAIR	Fat saturation/ water excitation/ SPAIR
Saturation regions	Regular/Parallel	Regular/Parallel
MTC	✓	✓
Phase partial Fourier	✓	–
Averaging mode	Long term	Long term
Multi-slice mode	Single-shot	Interleaved
Flow compensation	No	No
Dimension	2D	2D
RF pulse type	Normal	Normal/Low SAR
RF spoiling	Off	Off

	ep2d_diff	resolve
Gradient mode	Fast/Normal	Fast/Normal/ Whisper
b-value	0–10000	0–10000
Online reconstruction	DW and ADC image, FA image, TRACE	DW and ADC image, FA image, TRACE
iPAT	✓	✓
Multi-breathhold	✓	✓
2D PACE	Multi-breathhold/ Trigger	Multi-breathhold/ Trigger

^a parameter cannot be freely set, depends on base and phase resolution

^b parameter cannot be freely set, depends on other parameters

Perfusion Imaging: Sequence description

Prerequisites: Inline Perfusion and Neuro Perfusion Evaluation. The basic functionality is already included in the Tim Application Suite.

ep2d_fid

Single-shot FID EPI sequence.

Use

For perfusion imaging in the head. You can activate online reconstruction of the following images on the Perf parameter card:

- Time to Peak (TTP)
- Global Bolus Plot (GBP)
- Percentage of Baseline at Peak (PBP)

Recommendations. To minimize image distortions through susceptibility, select a bandwidth that enables use of minimum echo spacing.

	ep2d_fid
EPI Factor ^a	1 – 256
TE variable	✓
Contrasts	1
Bandwidth variable	Min ... max
Magn. Preparation	–
Recon. mode	Magnitude
Fat suppression	Fat saturation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Averaging mode	Long term
Multi-slice mode	Single-shot
Flow compensation	No
Dimension	2D
RF pulse type	Normal
RF spoiling	Off
Gradient mode	Fast/Normal
b-value	–
Online reconstruction	TTP, GBP, PBP
iPAT	✓

^a parameter cannot be freely set, depends on base and phase resolution

BOLD Imaging: Sequence description (I)

Prerequisites: Inline BOLD Imaging. The basic functionality is already included in the Tim Application Suite (ep2d_fid).

ep2d_bold

Single-shot FID EPI sequence.

Use

For BOLD imaging in the head. t-test evaluation in real time during the measurement. The calculated t-test images are shown continuously in the online display.

gre_field_ mapping

2D gradient echo sequence that generates images at two different echo times. The first TE is variable, the second TE is fixed relative to the first TE. The different echo times correspond to the in-phase conditions of fat and water protons.

Use

When phase images are selected, you obtain a single phase differential image that can be used as a “Fieldmap” during BOLD post-processing. The information is required when overlaying anatomical images generated with other techniques, e.g., SE or MPAGE.

Prerequisites for using the BOLD post-processing card:

- Image geometry and slice orientation have to be identical to the EPI images
- The sequence has to be applied prior to the corresponding EPI measurement

Note. These limitations do not apply when using the 3D Neuro card.

BOLD Imaging: Parameter ranges

	ep2d_bold	gre_field_mapping
EPI Factor ^a	1–128	
TE variable	✓	✓
Contrasts	1	2
Bandwidth variable	Min...max	✓
Magn. Preparation	–	–
Reconstruction mode	Magnitude	Magnitude/Phase
Fat suppression	Fat saturation	Fat saturation
Saturation regions	Regular/Parallel	Regular/Parallel/ Tracking
MTC	✓	✓
Phase Partial Fourier	✓	✓
Asymm. Echo	–	✓
Averaging mode	Long term	Short term/ long term
Multi-slice mode	Single-shot	Interleaved/sequen- tial
Flow compensation	No	Yes
Dimension	2D	2D
RF pulse type	Normal	Fast/Normal
RF spoiling	Off	On/off
Gradient mode	Fast	Fast/Normal/Whis- per

^a parameter cannot be freely set, depends on base and phase resolution

BOLD Imaging: Sequence description (II)

Prerequisites: Advanced Functional Neuro.

ep2d_pace

Identical to ep2d_bold, but with prospective 3D motion correction.

Note. By switching off motion correction, the entire function including prospective correction is deactivated.

	ep2d_pace
EPI Factor ^a	1 – 128
TE variable	✓
Contrasts	1
Bandwidth variable	Min...max
Magn. Preparation	–
Recon. mode	Magnitude
Fat suppression	Fat saturation/ water excitation
Saturation regions	Regular/Parallel
MTC	✓
Phase Partial Fourier	✓
Averaging mode	Long term
Multi-slice mode	Single-shot
Flow compensation	No
Dimension	2D
RF pulse type	Normal
RF spoiling	Off
Gradient mode	Fast

^a parameter cannot be freely set, depends on base and phase resolution

Application package Interactive Realtime: Sequence description

The Interactive Realtime package contains the BEAT_IRT sequence which has been optimized for interactive real-time imaging. *During* the measurement, all slice parameters can be changed via graphic slice positioning and the parameter cards.

(*Prerequisite:* Sequence is started via the **Stop/Continue** in the **Inline Display**).

The slice positions can be saved during imaging and subsequently transferred to a protocol in the wait queue.

BEAT_IRT is based on the CV sequence and inherits most of the parameter settings from it.

Sequence type	Fast sequence with a high signal-to-noise ratio.
Trufi	Use This sequence is very well suited for cardiac and abdominal applications.
Sequence type	Slower sequence with a lower SAR than Trufi.
Gre	Use This sequence is very well suited for interventional imaging; susceptibility effects enable a good view of biopsy needles.

Application package Interactive Realtime: Parameter ranges

Sequence type	Trufi
TE variable	— ^a
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	✓
Recon. mode	Magnitude
Fat suppression	—
Saturation regions	Regular
MTC	—
Phase Partial Fourier	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	No
Dimension	2D
RF pulse type	Fast/Normal/Low SAR
RF spoiling	Off
Gradient mode	Fast/Normal/Whisper
Dark blood	✓
Trajectory	Cartesian
Slices	1


^a TE is automatically set to the minimum and cannot be changed

Sequence type	Gre
TE variable	✓
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	✓
Recon. mode	Magnitude
Fat suppression	Fat saturation/ water excitation
Saturation regions	Regular
MTC	–
Phase Partial Fourier	✓
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	Yes/no
Dimension	2D
RF pulse type	Fast/Normal/Low SAR
RF spoiling	On/Off
Gradient mode	Fast/Normal/Whisper
Dark blood	✓
Trajectory	Radial
Slices	1

Application package

Susceptibility-Weighted Imaging (SWI)

Venous vessels as well as hemorrhages in the human brain may be displayed with susceptibility-weighted imaging. For this purpose, the different magnetic characteristics of deoxygenated blood and normal brain tissue are used.

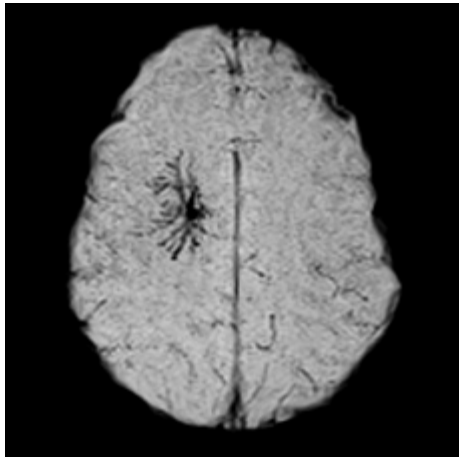

Method

For data acquisition, a high-resolution 3D gradient echo sequence with echo times of 40 ms at a field strength of 1.5 T or 20 ms at 3 T is used. Using the long echo times, the MR signals in venous blood and normal brain tissue are able to create a phase difference. This phase difference is used for contrasting where veins and hemorrhages are shown as dark.

Image reconstruction

Two image series are computed In the **Magnitude** reconstruction mode:


- MIP reconstructions of the SWI images across eight slices each (Sliding Window mode)
- SWI images without MIP reconstruction

In the **Magnitude/Phase** reconstruction mode, two more are computed in addition to the above mentioned image series:

- Conventional magnitude images
- Phase images

Application package BLADE: Application/sequence description

The BLADE technique helps reduce the motion sensitivity of MR examinations. BLADE is available for the tse sequence.

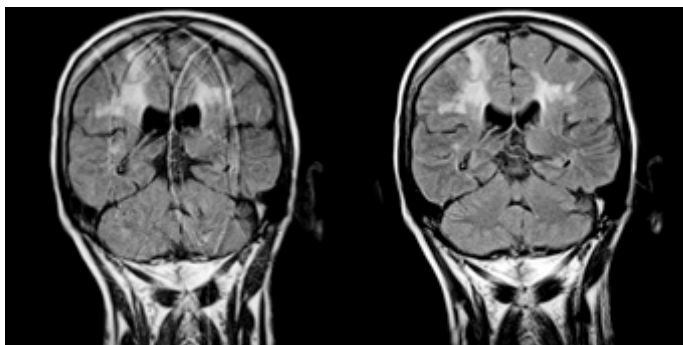

left: without BLADE; right: with BLADE


Use

- improves image quality in case of uncooperative patients
- T1-, T2- weighting, STIR, dark fluid
- respiratory-triggered, abdominal measurements with 2D PACE

**Sequence
description**

When using the BLADE technique, each echo train of the sequence generates a low-resolution image. The phase-encoding direction of this image is turned from one excitation to the next. Subsequently, the individual, low-resolution images are combined into a high-resolution image.

*Sampling of
the k-space
with BLADE:
Each echo train
fills an
individual
stripe, the
so-called blade*

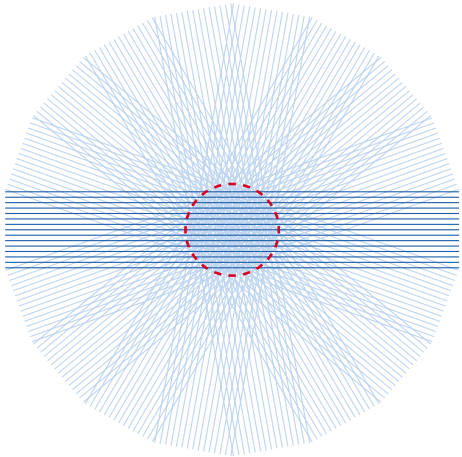


Example: Coverage of the k-space by 9 BLADES that contain 15 phase encoding lines each. The center of the k-space (red circle) is sampled again with each blade.

Application package BLADE: Sequence parameters

In the **Resolution/Common** parameter card

- Trajectory: BLADE
- BLADE coverage: determines the number of blades with different rotation angles
 - 100%:** the circle in the k-space is completely filled
 - > 100%:** the blades overlap the SNR improves
 - < 100%:** the k-space is not completely covered; shorter measurement time, however, poorer image quality

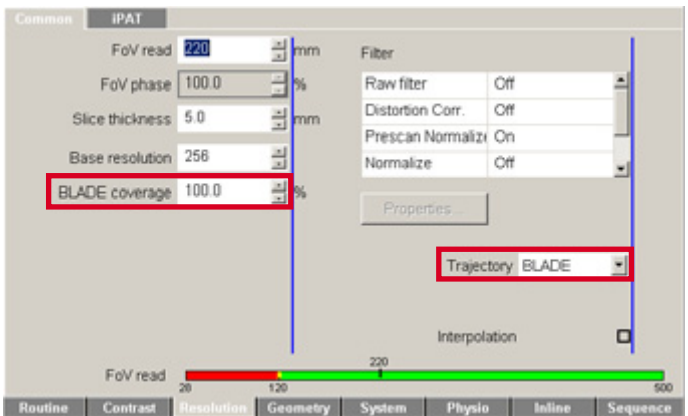

In the **Sequence/Part 2** parameter card

- Turbo factor: number of lines per blade (if GRAPPA is not used)
- Motion correction On:
Corrects patient motion within the image plane (in-plane) which happens between the acquisition of two blades

Use motion correction only for rigid body motion (e.g., at the head), but not for abdominal imaging, for example.

The screenshot displays the 'Sequence/Part 2' parameter card in an MRI software interface. The card is divided into two main sections by a vertical blue line. On the left, under the 'Define' tab, the 'Turbo factor' is set to 35 and 'Echo trains per slice' is set to 11. On the right, 'RF pulse type' and 'Gradient mode' are both set to 'Fast'. Below these, 'Motion correction' is set to 'On', and 'Stereotactic' is set to 'On'. A red box highlights the 'Turbo factor' field, and another red box highlights the 'Motion correction' dropdown menu. At the bottom of the card, there is a row of tabs: 'Routine', 'Contrast', 'Resolution', 'Geometry', 'System', 'Physio', 'Inline', and 'Sequence'.

Part 1	Part 2
Define	Turbo factor
Turbo factor	35
Echo trains per slice	11
RF pulse type	Fast
Gradient mode	Fast
Motion correction	On
Stereotactic	On

Routine Contrast Resolution Geometry System Physio Inline Sequence

Application package BLADE:


Application notes

1. To use BLADE as trajectory, the turbo factor has to be ≥ 9 .
2. To use motion correction, the turbo factor has to be ≥ 28 .
3. The accuracy of the BLADE reconstruction depends on the turbo factor. This is why BLADE protocols have a higher turbo factor and shorter echo spacing than a conventional TSE protocol with the same echo time.
4. For matrix sizes up to 320 and without GRAPPA, the images are usually available immediately or shortly after the measurement. Larger matrix sizes or the use of GRAPPA delay image reconstruction.
5. When using GRAPPA, the number of reference lines has to be considerably lower than the turbo factor (typically 8–12 as compared to 24 for conventional TSE imaging).

5. The *true* FOV of the sequence is *not* displayed. It corresponds to the blue circle in the square FoV (visible with graphic slice positioning). In the figure, the true expanded FoV (with phase-oversampling) is shown as a green circle. Due to the different phase-encoding directions of the individual blades, anatomy outside the true expanded FoV is aliased.

Avoiding aliasing. Use phase-oversampling.

Use phase-oversampling to avoid aliasing of the neck. The elements of the neck coil should not be selected.

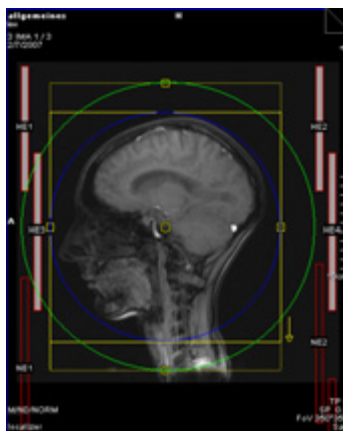

tse Dixon: Application

tse Dixon is a water-fat separation technique based on the 2D tse sequence. The Dixon technique can be used as an alternative to FatSat.

Use

- T1, T2, and PD weighting
- Compatible with multi-coil acquisition and iPAT (GRAPPA)

Advantages

- Up to four contrasts are possible within one measurement (in-phase, opposed-phase, water, and fat images)
- Less sensitive to B0 and B1 inhomogeneities
- Improved outcome with MR Conditional implants^a

^a Please adhere to all safety instructions regarding implants (-> Operator Manual - MR System)

Image examples:

top left: reliable FatSat

top right: with MR Conditional implants

bottom left: fat image

bottom right: water image



tse Dixon: Sequence description/ sequence parameters

Sequence description


As compared to conventional se or tse sequences, an opposed-phase gradient echo is acquired besides the original in-phase spin echo. The echoes are obtained at the time when the phase shift between water and lipid is " $-\pi$ " or " 0 ", respectively. After a linear combination of the images with phase correction, water and fat selective images can be computed.

In the **Contrast/Common** parameter card

Dixon	Determines whether fat and water images are displayed separately
None	Dixon method is not applied
Water + fat	Dixon method is performed and two images are reconstructed: one image contains only the water signal, the other only the fat signal
Save original images	Saves also in-phase and opposed-phase images besides separated water and fat images

Application package SPACE: Application

- Neuro imaging**
- Brain: isotropic resolution
 - Brain: Measurements with thicker, contiguous slices
 - Inner ear: High resolution
 - Spine: in place of several 2D acquisitions

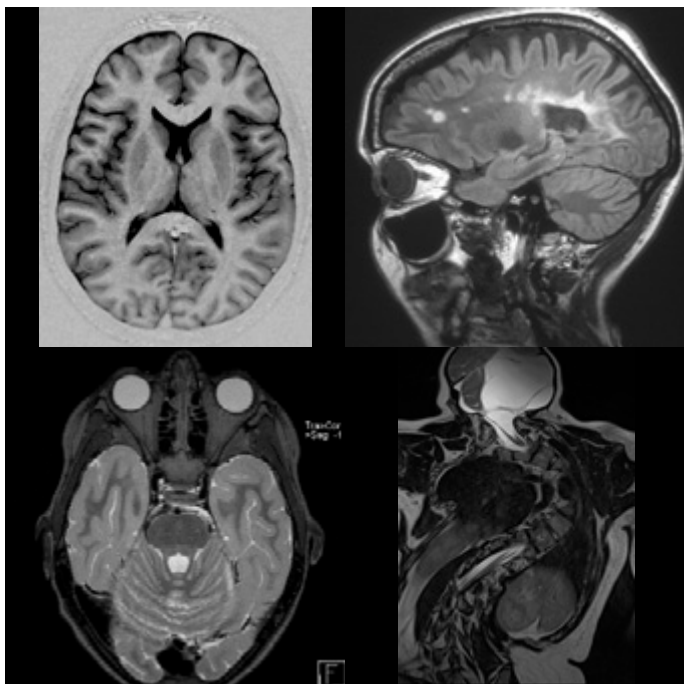

- Body imaging**
- Pelvis: in place of several 2D acquisitions
 - PACE MRCP during free breathing
- Ortho imaging**
- PD and T1 weighting with isotropic, high-spatial resolution (with or without fat suppression)



Application package SPACE: Sequence description/protocols

The SPACE sequence is a variant of the 3D Turbo spin echo sequence (tse_vfl). As compared to a conventional TSE sequence, SPACE uses non-selective, short refocusing pulse trains that consist of excitation pulses with variable flip angles. This allows for very high turbo factors (>100) and high sampling efficiencies. As a result, you obtain high-resolution, isotropic images that allow free reformats in all planes.

Optimized protocols

The following applications in the Siemens protocol tree include optimized SPACE protocols:

- Head: T1, T2, dark fluid, Double Inversion Recovery, and TrueIR contrast
- Spine: T2 contrast
- Body: T2 contrast, MRCP
- Ortho: PD and T1 contrast (with and without fat suppression)

Application package SPACE: Sequence parameters

In the **Sequence/Part 2** parameter card

- Turbo factor:
Number of RF refocusing pulses along the echo train
- Slice turbo factor:
Number of slices per echo train
- Echo trains per slice:
Number of echo trains per slice
(1 = single-shot,
>1 = segmented acquisition)
- Echo train duration:
Total duration depending on turbo factor, slice turbo factor and echo spacing
- Non-selective excitation:
Excitation and refocusing pulses
- Selective excitation:
Excitation pulse is slice-selective, refocusing pulses are non-selective, number of averages = 2 with phase cycling to reduce artifacts, uneven number of averages possible to reduce the measurement time, that is, averaging only across the central phase-encoding lines

Flip angle mode

Constant	Constant flip angle across the entire echo train. For heavily T2-weighted images (e.g., inner ear, MRCP) or PD- and T2-weighted imaging of the body.
PD var	Variable flip angle across the echo train. For short echo times.
T2 var	Variable flip angles across the echo train that affect strong dephasing of the flowing spins (dark blood, suppresses flow artifacts) and a low SAR. For T2 and dark fluid head imaging. To obtain T2 contrast comparable to that obtained with a conventional TSE sequence, a longer effective echo time has to be used.

The screenshot shows a software interface for configuring an MRI sequence. It is divided into 'Part 1' and 'Part 2' tabs. Under 'Part 1', there is a 'Define' dropdown set to 'Echo trains', and several numerical input fields: 'Turbo factor' (159), 'Slice turbo factor' (2), 'Echo trains per slice' (1), and 'Echo train duration' (850). Under 'Part 2', there are dropdown menus for 'RF pulse type' (Normal), 'Gradient mode' (Fast), 'Excitation' (Non-sel.), and 'Flip angle mode'. The 'Flip angle mode' dropdown is open, showing three options: '<<Constant>>', '<<PD var>>', and 'T2 var', with 'T2 var' currently selected. At the bottom, there is a horizontal bar with tabs labeled 'Routine', 'Contrast', 'Resolution', 'Geometry', 'System', 'Physio', 'Inline', and 'Sequence'.

Application package TimCT Angiography: Sequence description

The TimCT angiography package enables examinations of large body areas with continuous table move. The otherwise necessary measurement pauses, where the patient table is moved from one stage to the next, are no longer necessary. The result is a uniform image quality in the direction of the table move.

Please note: The table movement renders some conventional settings unsuitable, e.g., tilting of the slice block from the movement axis of the table or several averages.

fl3d_ce_ct

Gradient echo sequence.

Use

Optimized for CE angiography of the peripheral vessels with continuous table move.

	fl3d_ce_ct
Segments	1
TE variable	Min.
Contrasts	1
Bandwidth variable	✓
Magn. Preparation	–
Reconstruction mode	Magnitude
Fat suppression	–
Saturation regions	–
MTC	–
Phase Partial Fourier	✓
Asymm. Echo	Allowed
Flow compensation	No
Dimension	3D
Elliptical scanning	✓
Slice resolution	✓
Slice Partial Fourier	✓
Excitation pulse	Slab-selective
RF pulse type	Fast/Normal
RF spoiling	On
Gradient mode	Fast/Normal
CARE Bolus	–
iPAT	✓
iPAT ²	–
Variable resolution	✓

MR thermometry: Sequence description

ep_seg_therm	Segmented, temperature-sensitive EPI sequence. With an EPI factor of 1, the sequence behaves like a gre sequence. Use For displaying large changes in temperature ($\geq 15\text{ }^{\circ}\text{C}$) in tissue. Additional information for MR thermometry is included in the <i>Body Imaging Application Brochure</i>.
---------------------	--

	ep_seg_therm
EPI Factor	1
TE variable	–
Contrasts	1
Bandwidth variable	–
Magn. Preparation	–
Reconstruction mode	Magnitude/Phase
Fat suppression	–
Phase Partial Fourier	–
Asymm. Echo	Off
Averaging mode	Short term
Multi-slice mode	Sequential
Flow compensation	–
Dimension	2D
Excitation pulse	Slice-selective
RF pulse type	Normal
RF spoiling	On
Gradient mode	Fast
iPAT	–
Trajectory	Cartesian
Slices	1

© Siemens Healthcare GmbH, 2017
Print No. MR-07015G.643.44.02.02

www.siemens.com/healthcare